



Calibration results summary

Points with s/c potential between 1.97 - 2.03V

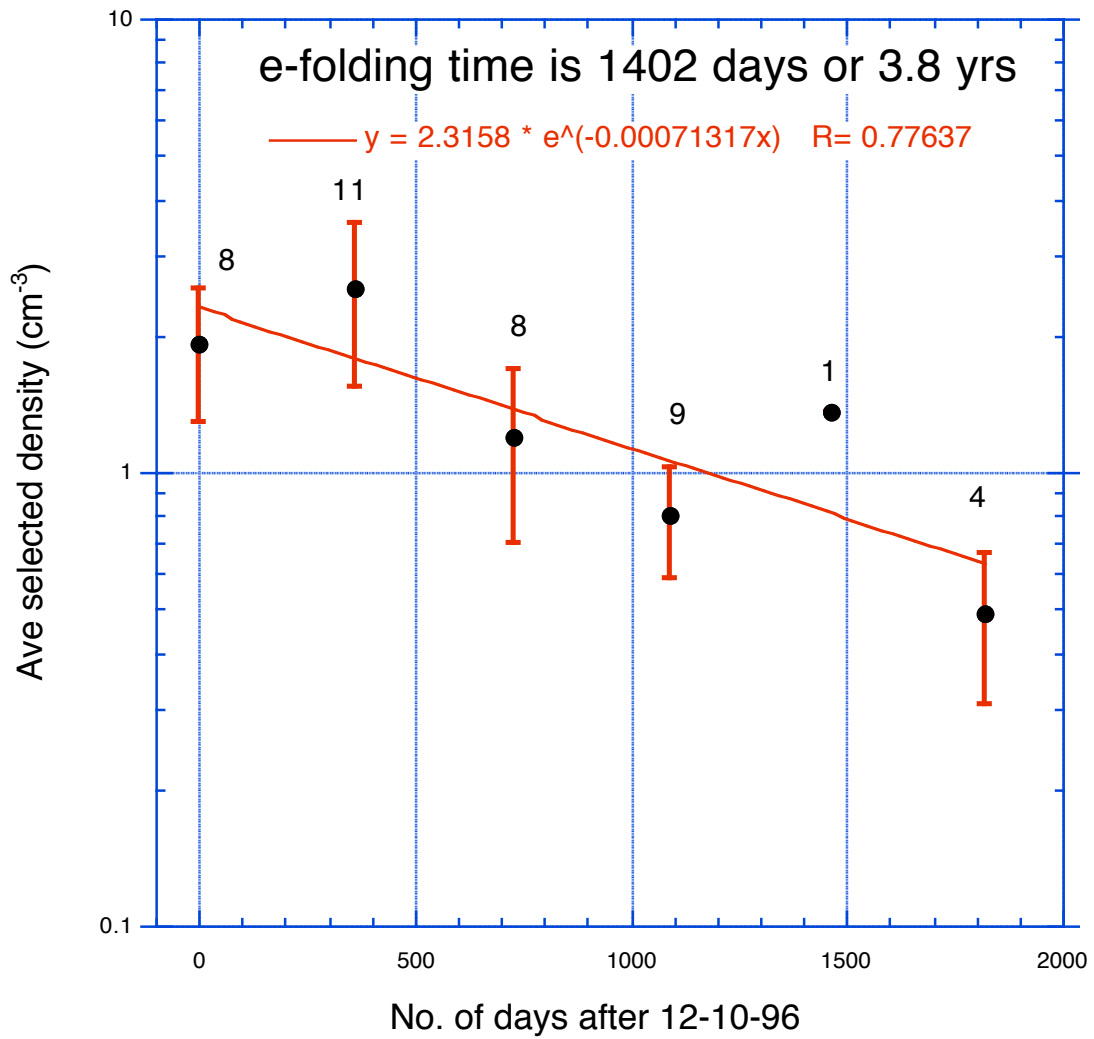

Calibration results summary

Points with s/c potential between 1.45 - 1.55V

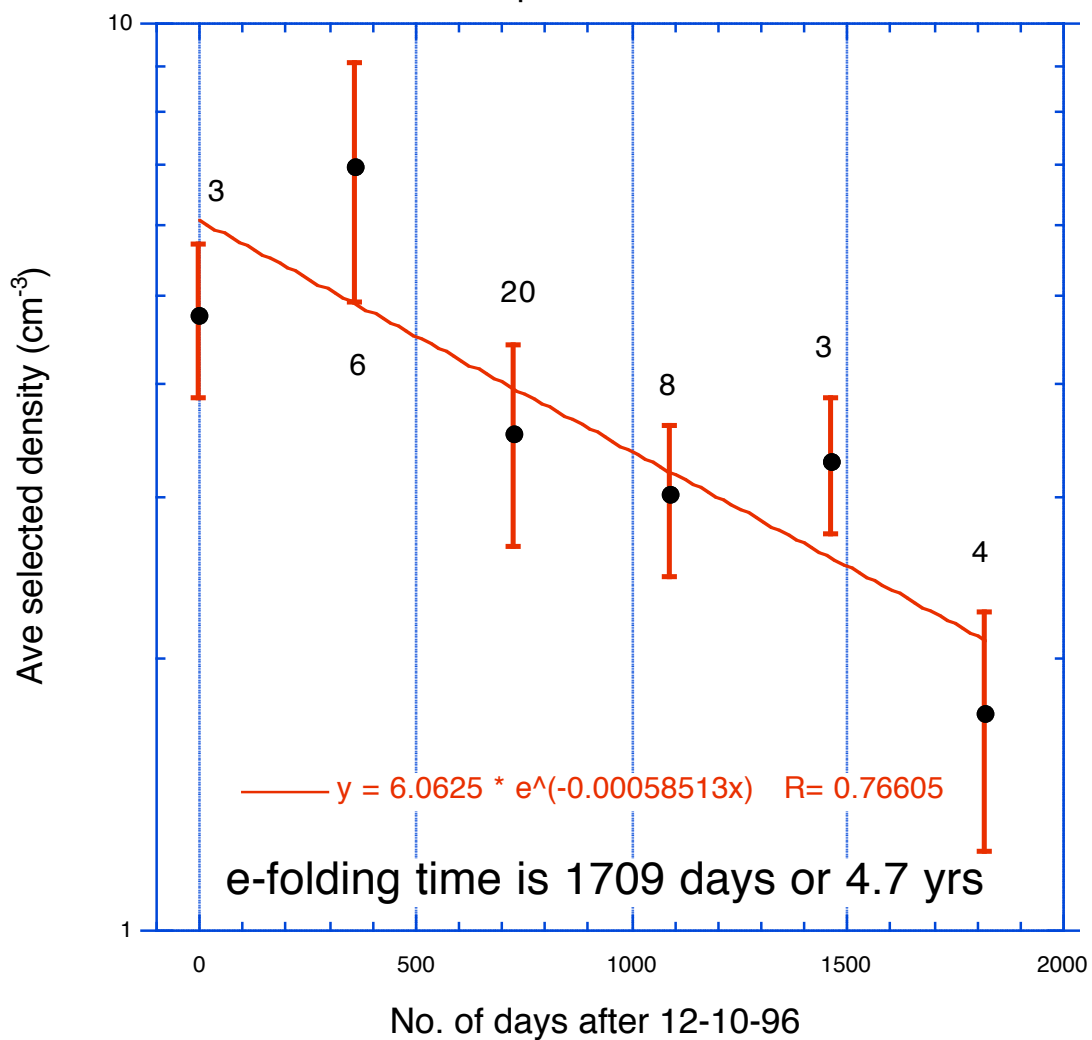

Summary of results of average
densities for $1.95 < \rho_{sc} < 2.05V$
(12/10/96 - 12/7/02)

